
000111110001

Cascade Impedance Standard SubstrateMap

> P/N: 143-033

Pitch: **100 μm - 250 μm** Configuration: **GSG**




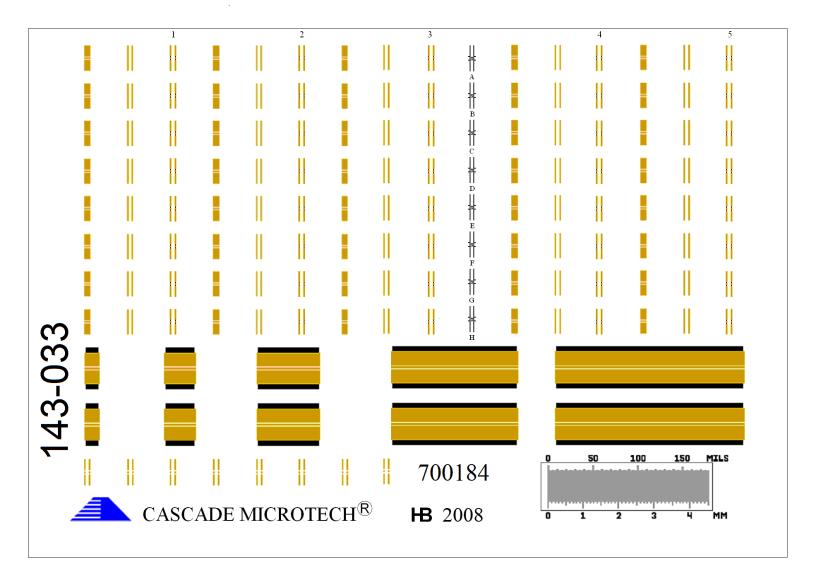


Key to Map

Key to the 143-033 Map

Substrate specifications: Material: Alumina; Thickness: 10 mils (254 um); Dielectric constant: 9.9

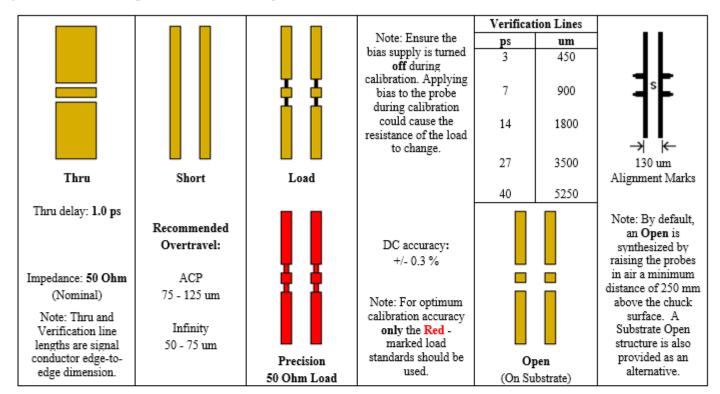

All of the above specifications are based on an overtravel (downward movement of probe after initial touchdown on the substrate) listed above. This amount of overtravel can be set before calibration on the Impedance Standard Substrate (ISS) using the alignment marks (allows precise setting of probe separation and overtravel). Figure 1 shows that initial contact with the edge of the probe tips should be made at reference plane X. The desired overtravel and thus skate (forward movement of probe tips after initial contact with substrate) is then achieved by adjusting the Z height on the positioner to move the edge of the probe tips to reference plane Y. This can also be seen from the images shown in Figure 2.



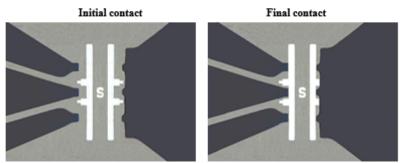


Figure 2: Images showing correct alignment and placement of probe tips of both ACP and Infinity style probes.

Calibration Coefficients are dependent on the probe tip configuration, placement on a standard, and the standard configurations. This leads to unique calibration coefficients for a unique pair of probe and ISS. Therefore, the calibration coefficients are supplied with the probe not with the ISS.

© Copyright 2020 FormFactor, Inc. All rights reserved. FormFactor and the FormFactor logo are trademarks of FormFactor, Inc. All other trademarks are the property of their respective owners. All information is subject to change without notice. Corporate Headquarters 7005 Southfront Road Livermore, CA 94551 Phone: 925-290-4000 www.formfactor.com

Document PN: 146-587 rev 2

