

# Tesla 300 mm Probe System

This guide contains information to help prepare your facility for the arrival of your FormFactor probe station.



**DANGER**

FormFactor requires that the light curtain safety interlock is installed prior to use of this equipment. The interlock must be active whenever high voltage is present. Customers are responsible for ensuring proper connection and that the safety interlock is active before use.



**NOTE**

Facility requirements for thermal systems are listed separately. See the Facility Planning Guide specific to your thermal system for details.

## Probe Station Requirements

Clean Dry Air (CDA)	General use	<ul style="list-style-type: none"> <li>• ISO 8573.1 Class 1.4.1 (3°C dew point, oil less than 0.01 mg/m<sup>3</sup>)</li> <li>• 85 l/min (3 CFM) at SATP* supplied at 6-8 bar (87 - 116 psi) gauge</li> <li>• 12.7 mm (1/2 in) OD push-in tube connection (3 m max tube length)</li> </ul>
	MicroChamber probing environment	<ul style="list-style-type: none"> <li>• ISO 8573.1 Class 1.1.1 (-70°C dew point, oil less than 0.01 mg/m<sup>3</sup>)</li> <li>• Max flow: 170 l/min (6 CFM) at SATP* supplied at 6-8 bar (87 - 116 psi) gauge</li> <li>• Continuous flow: 57-85 l/min (2-3 CFM) at SATP* supplied at 6-8 bar (87 - 116 psi) gauge</li> <li>• 12.7 mm (1/2 in) OD push-in tube connection (3 m max tube length)</li> </ul>
	MicroChamber probing environment and general use CDA	<ul style="list-style-type: none"> <li>• ISO 8573.1 Class 1.1.1 (-70°C dew point, oil less than 0.01 mg/m<sup>3</sup>)</li> <li>• Max flow: 255 l/min (9 CFM) at SATP* supplied at 6-8 bar (87 - 116 psi) gauge</li> <li>• Continuous flow: 57-85 l/min (2-3 CFM) at SATP* supplied at 6-8 bar (87 - 116 psi) gauge</li> <li>• 12.7 mm (0.5 in.) OD push-in tube connection (max 3 m tube length)</li> <li>• Chamber atmospheric pressure dew point:                             <ul style="list-style-type: none"> <li>– Thermal system operated down to +20°C: ≤ -45°C at SATP* (-29°C at 5 bar [73 psi] gauge)</li> <li>– Thermal system operated down to -40°C: ≤ -50°C at SATP* (-35°C at 5 bar [73 psi] gauge)</li> <li>– Thermal system operated down to -60°C: ≤ -70°C at SATP* (-57°C at 5 bar [73 psi] gauge)</li> </ul> </li> </ul> <p>CDA for general use may be supplied by the MicroChamber supply for a single service supply.</p>
	<p><b>WARNING</b></p> <p>FormFactor does not endorse or recommend using nitrogen instead of CDA for thermal system operation with any FormFactor system due to the risk of oxygen depletion in the working environment.</p> <p>If your testing configuration requires the use of nitrogen instead of CDA for MicroChamber purge, time in Quick Purge mode should be controlled. Discuss your setup with your safety and facilities departments to ensure that the oxygen flow in your working environment is adequate to dissipate any nitrogen build up. The use of oxygen sensor alarms is also recommended.</p>	
	<p><b>NOTE</b></p> <p>Note that the combined values for independent general use and MicroChamber purge flow are not equal to the value for simultaneous general use and MicroChamber purge flow.</p> <p>Modification of the manifold plumbing is required if you are using N<sub>2</sub>. See the Summit User Guide for details.</p>	
Vacuum	<ul style="list-style-type: none"> <li>• Wafer hold on chuck and positioners:                             <ul style="list-style-type: none"> <li>– Required: &lt; 500 mbar (14.8 inHg) absolute, -510 mbar (-15.0 inHg) gage, at up to 8 l/min (0.28 CFM) at SATP*</li> <li>– Recommended: &lt; 400 mbar (11.8 inHg) absolute, -610 mbar (-18.0 inHg) gage, at up to 10 l/min (0.35 CFM) at SATP*</li> <li>– 12.7 mm (0.5 in.) OD push-in tube connection (3 m max tube length)</li> </ul> </li> <li>• Wafer hold only (while under test to ensure measurement performance):                             <ul style="list-style-type: none"> <li>– Vacuum pressure stability: ± 10 mbar (0.3 inHg)</li> </ul> </li> </ul>	

# Tesla 300 mm Probe System

<b>Power</b>	Station	<ul style="list-style-type: none"> <li>• Single phase: 100-120 VAC or 200-240 VAC, 10 A, 50/60 Hz</li> <li>• Source (plugs): <ul style="list-style-type: none"> <li>– North America: NEMA 5-20 for 100-127 VAC or NEMA L6-15 for 208-240 VAC</li> <li>– Europe: CEE VII (Schuko)</li> <li>– Other: consult factory</li> </ul> </li> <li>• Appropriate international power cables will be supplied.</li> </ul>	
	Circuit breaker	<ul style="list-style-type: none"> <li>• Minimum rating: 10,000 AIC</li> </ul>	
	Accessories	<p>Up to four additional power outlets are available depending on the configuration and are rated at 115V/230V for accessories.</p> <hr/> <p>Power to the dual LCD computer monitors is supplied by the built-in power strip on the station.</p> <hr/> <p>Additional AC outlets required: 115V/230V for accessories</p> <ul style="list-style-type: none"> <li>• Test equipment</li> <li>• Laser system</li> <li>• Instrument/video monitors</li> <li>• Vacuum pump</li> </ul>	
<b>Thermal Systems</b>	Refer to the facility preparation guide for your thermal system. Note that the standard low temperature range is adjusted to -55°C due to complexity of the high voltage chuck.		
<b>Environmental Conditions</b>	Operating	<ul style="list-style-type: none"> <li>• Indoors only</li> <li>• Altitude up to 1000 m</li> <li>• Main supply voltage fluctuations not to exceed <math>\pm 10\%</math> of the nominal voltage</li> </ul>	
	Ambient temperature	<ul style="list-style-type: none"> <li>• +18°C to +28°C</li> </ul>	
	Relative humidity	<ul style="list-style-type: none"> <li>• 20% to 60%</li> </ul>	
	Ambient vibration (including floor)	<p>The probe station is intended for use in an environment having background vibrations at or below the ISO Operating Theatre level:</p> <ul style="list-style-type: none"> <li>• Maximum level 4000 micro-in./sec (72 dB), measured using the 1/3-octave-band velocity spectra method</li> </ul>	
	Seismic restraints	Installation of seismic restraints is required to safely restrain the probe station during a seismic event and to meet the safety requirements as outlined by SEMI-S2.	
<b>Dimensions</b>	See <a href="#">Dimensions</a> on page 3.		
	Additional clearance	Front	800 mm (31 inches) for operator/installation during installation or service
		Back	1000 mm (39 inches) for service access 800 mm (31 inches) when using optional holders for monitor, keyboard or test instrument
	Left/right	Left/right	200 mm (8 inches) for cables, maximum 450 mm for use of control console 800 mm (31 inches) during installation or service, or permanently when using optional holders for monitor, keyboard or test instrument
		Top	400 mm (16 inches)
Additional clearance may be required for thermal system cooling units.			
<b>Weight</b>	Probe station	<ul style="list-style-type: none"> <li>• ~1090 kg (2400 pounds)</li> </ul>	
	Lifting requirements	<ul style="list-style-type: none"> <li>• If the station is to be moved short distances, use the integrated wheels.</li> <li>• To move the probe station long distances, it must be in the original shipping crate and a forklift must be used. To avoid personal injury and/or damage to the probe station, a forklift with a minimum 1364 kg (3000 pound) capacity is required.</li> </ul>	
<b>Shipping Dimensions (WxDxH)</b>	Probe station	<ul style="list-style-type: none"> <li>• 1520 x 1520 x 1600 mm (60 x 60 x 63 inches)</li> </ul>	
<b>Shipping Weight</b>	Probe station	<ul style="list-style-type: none"> <li>• ~1295 kg (2850 pounds)</li> </ul>	

# Tesla 300 mm Probe System

\* Standard Ambient Temperature And Pressure (SATP)


## Dimensions



### NOTE

Refer to [Additional clearance](#) on page 2 for recommended working space around the station.


## Front View (Standard Height Option)

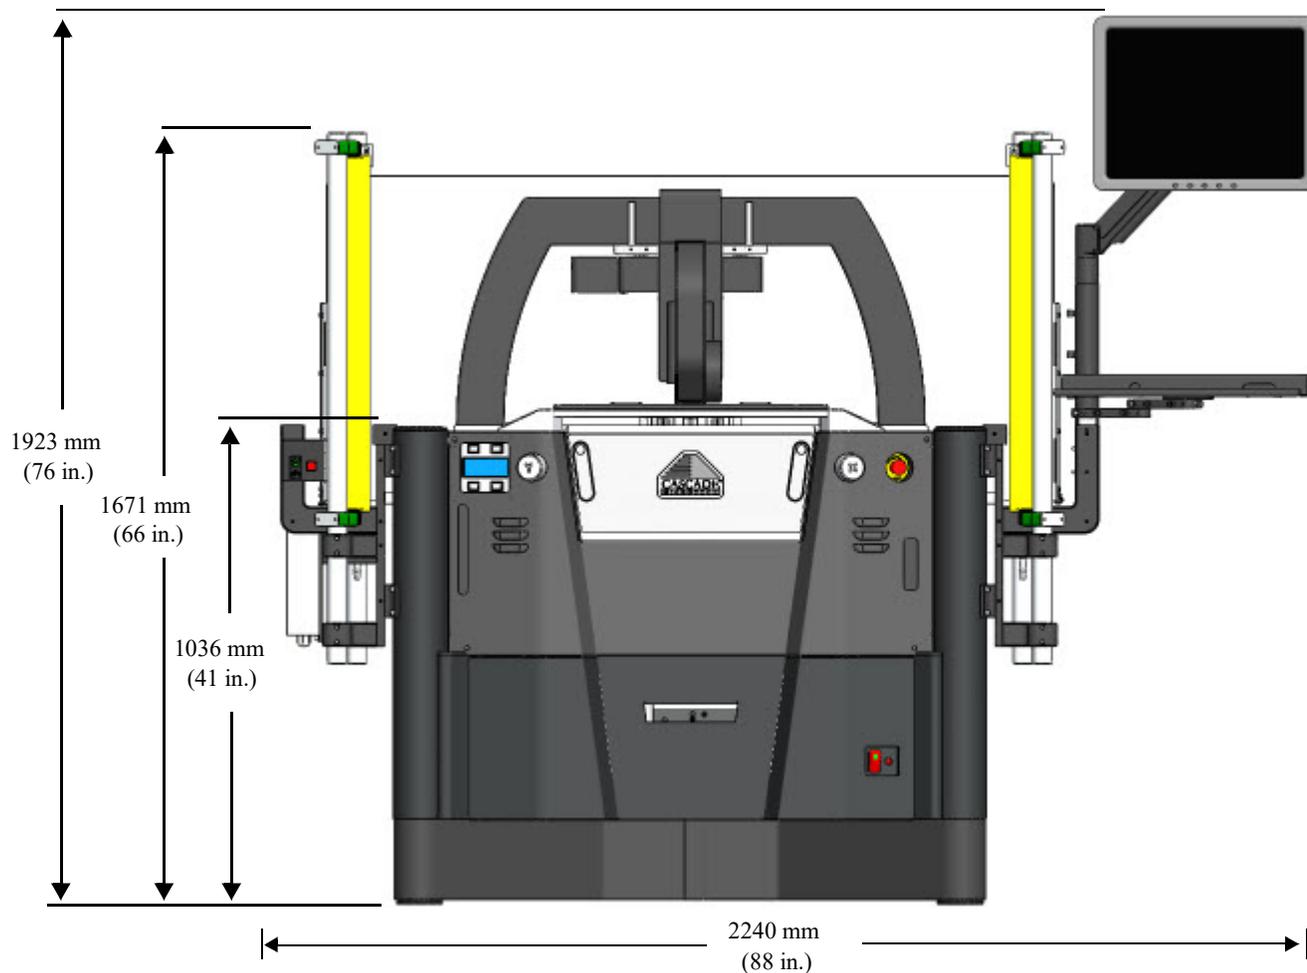

# Tesla 300 mm Probe System

---


## Side View

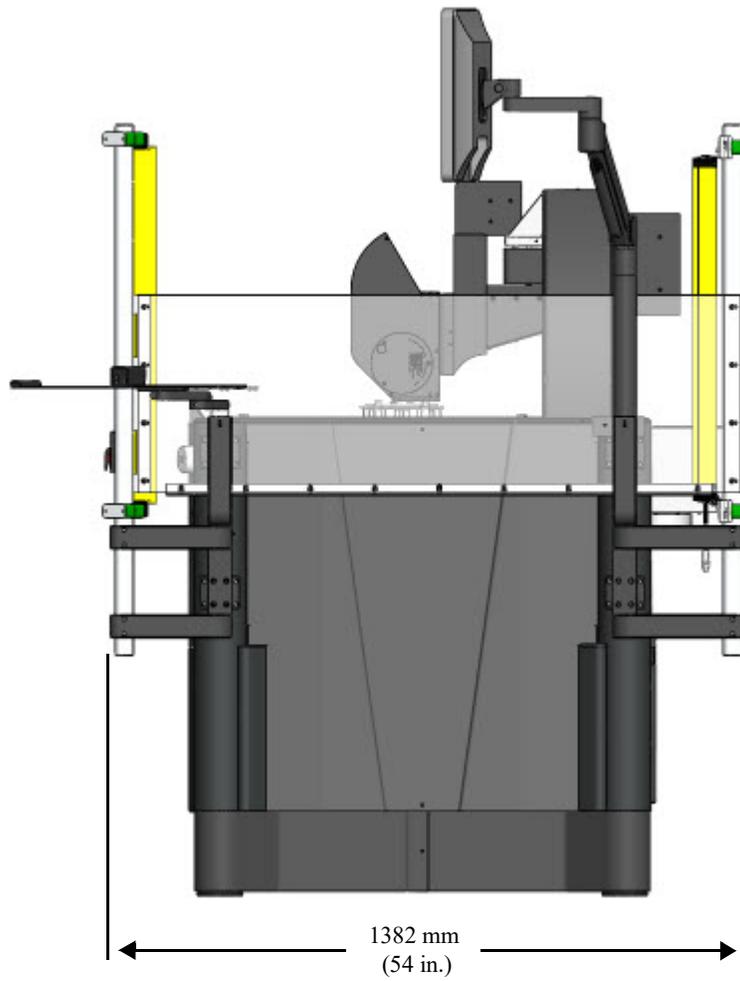

# Tesla 300 mm Probe System

---

## Top View

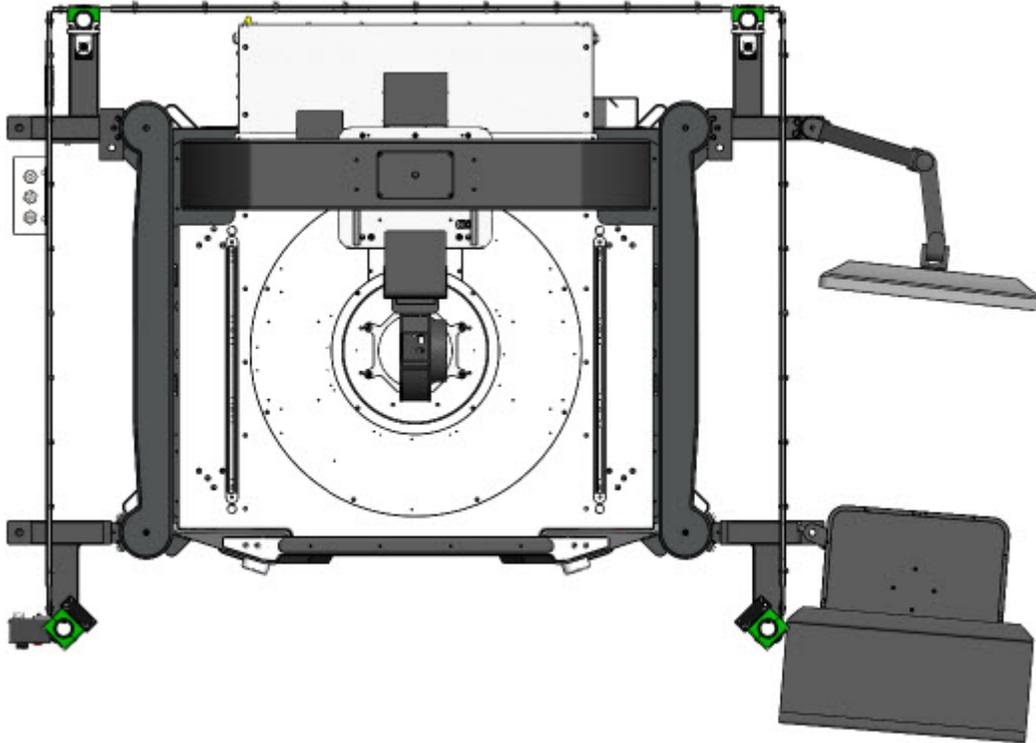

© Copyright 2018 FormFactor, Inc. All rights reserved. No part of this document may be reproduced, transmitted or displayed in any form or by any means except as duly authorized by FormFactor, Inc. FormFactor and the FormFactor logo are trademarks of FormFactor, Inc. All other trademarks are the property of their respective owners.

### Important Notice

While the information contained herein is believed to be accurate as of the date hereof, no express or implied representations or warranties are made with respect to its accuracy or completeness. FormFactor, Inc., and its subsidiaries disclaim liability for any inaccuracies or omissions. All information is subject to change without notice.

Users are required to read and follow carefully all safety, compliance and use instructions. Users assume all loss and liability arising from the use of products in any manner not expressly authorized. The conditions and methods of use of products and information referred to herein are the entire responsibility of the user and, to the maximum extent permitted by applicable law, FormFactor, Inc., and its subsidiaries shall not be liable for any damages, losses, costs or expenses arising out of, or related to, the use thereof.

No license, express or implied, by estoppel or otherwise, under any intellectual property right is granted in connection herewith. Users shall take all actions required to avoid intellectual property infringement.

### Corporate Headquarters

7005 Southfront Road  
Livermore, CA 94551  
Phone: 925-290-4000  
[www.formfactor.com](http://www.formfactor.com)

